



Standard Practice for Contact Ultrasonic Testing of Welds Using Phased Arrays¹

This standard is issued under the fixed designation E 2700; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice describes ultrasonic techniques for inspecting welds using phased array ultrasonic methods (see [Note 1](#)).

1.2 This practice uses angle beams, either in S-scan or E-scan modes, primarily for butt welds and Tee welds. Alternative welding techniques, such as solid state bonding (for example, friction stir welding) and fusion welding (for example, electron beam welding) can be inspected using this practice provided adequate coverage and techniques are documented and approved. Practices for specific geometries such as spot welds are not included. The practice is intended to be used on thicknesses of 9 to 200 mm (0.375 to 8 in.). Greater and lesser thicknesses may be tested using this standard practice if the technique can be demonstrated to provide adequate detection on mockups of the same wall thickness and geometry

1.3 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.4 *The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.*

NOTE 1—This practice is based on experience with ferrous and aluminum alloys. Other metallic materials can be examined using this practice provided reference standards can be developed that demonstrate that the particular material and weld can be successfully penetrated by an ultrasonic beam.

NOTE 2—For additional pertinent information, see Practices [E 2491](#), [E 317](#), and [E 587](#).

2. Referenced Documents

2.1 ASTM Standards:²

- [E 164 Practice for Contact Ultrasonic Testing of Weldments](#)
- [E 317 Practice for Evaluating Performance Characteristics of Ultrasonic Pulse-Echo Testing Instruments and Systems](#)

¹ This practice is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.06 on Ultrasonic Method.

Current edition approved Aug. 1, 2009. Published August 2009.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[without the Use of Electronic Measurement Instruments](#)
[E 543 Specification for Agencies Performing Nondestructive Testing](#)

[E 587 Practice for Ultrasonic Angle-Beam Examination by the Contact Method](#)

[E 1316 Terminology for Nondestructive Examinations](#)

[E 2192 Guide for Planar Flaw Height Sizing by Ultrasonics](#)

[E 2491 Guide for Evaluating Performance Characteristics of Phased-Array Ultrasonic Testing Instruments and Systems](#)

2.2 *ASME Standard:*³

ASME B and PV Code Section V, Article 4

2.3 *ISO Standard:*⁴

ISO 2400 Reference Block for the Calibration of Equipment for Ultrasonic Examination

2.4 *ASNT Documents:*⁵

[SNT-TC-1A Recommended Practice for Personnel Qualification and Certification in Nondestructive Testing](#)

[ANSI/ASNT CP-189 Standard for Qualification and Certification of NDT Personnel](#)

2.5 *AIA Standard:*⁶

[NAS-410 Certification and Qualification of Nondestructive Testing Personnel](#)

3. Terminology

3.1 *Definitions*—For definitions of terms used in this practice, see Terminology [E 1316](#).

4. Summary of Practice

4.1 Phased arrays are used for weld inspections for numerous applications. Industry specific requirements have been developed to control the use of this technology for those applications. A general standard practice document is required to define the requirements for wider use of the technology. Several manufacturers have developed portable, user-friendly

³ Available from American Society of Mechanical Engineers (ASME), ASME International Headquarters, Three Park Ave., New York, NY 10016-5990, <http://www.asme.org>.

⁴ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

⁵ Available from American Society for Nondestructive Testing (ASNT), P.O. Box 28518, 1711 Arlingate Ln., Columbus, OH 43228-0518, <http://www.asnt.org>.

⁶ Available from Aerospace Industries Association of America, Inc. (AIA), 1000 Wilson Blvd., Suite 1700, Arlington, VA 22209-3928, <http://www.aia-aerospace.org>.

instruments. Codes and code cases have been developed, or are being developed, to cover phased array weld inspection requirements by organizations such as ASME. Practice E 2491 covers setting up of phased arrays for weld inspections. Training programs for phased arrays have been set up worldwide. This practice provides procedural guidance for both manual and mechanized scanning of welds using phased array systems.

5. Significance and Use

5.1 Industrial phased arrays differ from conventional monocrystal ultrasonic transducers since they permit the electronic control of ultrasound beams. The arrays consist of a series of individual transducer elements, each separately wired, time-delayed and electrically isolated; the arrays are typically pulsed in groups to permit “phasing,” or constructive-destructive interference.

5.2 Though primarily a method of generating and receiving ultrasound, phased arrays are also a method of scanning and imaging. While some scan patterns emulate manual technology, other scans (for example, S-scans) are unique to phased arrays. With their distinct features and capabilities, phased arrays require special set-ups and standardization, as addressed by this practice. Commercial software permits the operator to easily make set ups without detailed knowledge of the phasing requirements.

5.3 Phased arrays can be used in different ways: manual or encoded linear scanning; and different displays or combinations of displays. In manual scanning, the dominant display will be an S-scan with associated A-scans. S-scans have the advantage over E-scans that all the specified inspection angles can be covered at the same time.

5.4 The main advantages of using phased arrays for ultrasonic weld examinations are:

5.4.1 Faster scanning due to multiple angles on display at the same time,

5.4.2 Better imaging from the true depth S-scan,

5.4.3 Data storage, for example, selected reflectors, for auditing, and archiving.

5.4.4 Rapid and reproducible set-ups with electronic instruments.

5.5 All personnel responsible for carrying out examinations, analysis and reporting results using this standard should be appropriately trained and qualified in accordance with a nationally or internationally recognized NDT personnel qualification practice or standard such as ANSI/ASNT CP-189, SNT-TC-1A, NAS-410, or a similar document and certified by the employer or certifying agency, as applicable. Additionally, there should also be training or knowledge and experience related to phased array equipment and techniques. Personnel performing examinations to this standard should list the qualifying credentials in the examination report.

6. Basis of Application

6.1 The following items are subject to contractual agreement between the parties using or referencing this standard.

6.2 *Personnel Qualification*—If specified in the contractual agreement, personnel performing examinations to this standard shall be qualified in accordance with a nationally or interna-

tionally recognized NDT personnel qualification practice or standard such as ANSI/ASNT CP-189, SNT-TC-1A, NAS-410, or a similar document and certified by the employer or certifying agency, as applicable. The practice or standard used and its applicable revision shall be identified in the contractual agreement between the using parties.

6.3 *Qualification of Nondestructive Agencies*—If specified in the contractual agreement, NDT agencies shall be qualified and evaluated as described in Practice E 543. The applicable edition of Practice E 543 shall be specified in the contractual agreement.

6.4 *Procedures and Techniques*—The procedures and techniques to be used shall be as specified in the contractual agreement. Practice E 2491 recommends methods of assessing performance characteristics of phased array probes and systems.

6.5 *Surface Preparation*—The pre-examination surface preparation criteria shall be in accordance with 9.1 unless otherwise specified.

6.6 *Timing of Examination*—The timing of examination shall be determined by the contracting parties and in accordance with the stage of manufacture or in-service conditions.

6.7 *Extent of Examination*—The extent of examination shall be suitable to examine the volume of the weld plus the heat affected zone unless otherwise specified.

6.8 *Reporting Criteria/Acceptance Criteria*—Reporting criteria for the examination results shall be in accordance with 13.1, unless otherwise specified. Since acceptance criteria are not specified in this standard, they shall be specified in the contractual agreement.

6.9 *Reexamination of Repaired/Reworked Items*—Reexamination of repaired/reworked items is not addressed in this standard and if required shall be specified in the contractual agreement.

7. Equipment

7.1 *Phased Array Instruments:*

7.1.1 The ultrasonic phased array instrument shall be a pulse echo type and shall be equipped with a standardized dB gain or attenuation control stepped in increments of 1 dB minimum, containing multiple independent pulser/receiver channels. The system shall be capable of generating and displaying both B-scan and S-scan images, which can be stored and recalled for subsequent review.

7.1.2 The phased array system shall have on-board focal law generation software that permits direct modification to ultrasonic beam characteristics. Specific delay calculations may be performed by the system itself or imported from external calculations.

7.1.3 The phased array system shall have a means of data storage for archiving scan data. An external storage device, flash card or USB memory stick can be used for data storage. A remote portable PC connected to the instrument may also be used for this purpose. If instruments do not inherently store A-scan data, such as some manual instruments, the final image only may be recorded.

7.1.4 The phased array system shall be standardized for amplitude and height linearity in accordance with Practice E 2491 annually, as a minimum.

7.1.5 The instrument shall be capable of pulsing and receiving at nominal frequencies of 1 MHz to 10 MHz. For special applications, frequencies up to 20 MHz can be used, but may require special instrumentation with appropriate digitization, and special approval.

7.1.6 The instrument shall be capable of digitization of A-scans at a minimum of five times the nominal frequency of the probe used. Amplitude shall be digitized at a resolution of at least 8-bit (that is, 256 levels).

7.1.7 The instrument shall be capable of equalizing the amplitude response from a target at a fixed soundpath for each angle used in the technique (angle corrected gain (ACG) thereby providing compensation for wedge attenuation variation and echo-transmittance).

7.1.8 The instrument shall also be equipped with facilities to equalize amplitudes of signals across the time-base (time-corrected gain).

7.2 *Phased Array Probes:*

7.2.1 The application requirements will dictate the design of the phased array probe used. Phased array probes may be used with a removable or integral wedge, delay-line, or in an immersion or localized bubbler system mode. In some cases a phased array probe may be used without a refracting wedge or delay-line (that is, just a hard wear-face surface).

7.2.2 Phased array probes used for weld examination may be of 1D, 1.5D or 2D design. Only 1D arrays or dual arrays configured with side-by-side transmitter-receiver arrays (as in Transmit-Receive Longitudinal wave probes) shall be used with manual scanning techniques. For 2D arrays, which use electronic oscillation, calibration should be performed at all skewed angles.

7.2.3 The number of elements in the phased array probe and the element dimensions and pitch shall be selected based on the application requirements and the manufacturer's recommended limitations.

7.2.4 The probe selected shall not have more elements than the number of elements addressable by the pulser-receivers available in the phased array instrument being used.

7.2.5 When refracting wedges are used to assist beam steering, the natural incident angle of the wedge shall be selected such that the angular sweep range of the examination technique used does not exceed the manufacturer's recommended limits for the probe and mode (compression or transverse) used.

7.2.6 Refracting wedges used on curved surfaces shall require contouring to match the surface curvature if the curvature causes a gap between the wedge and examination surface exceeding 0.5 mm (0.020 in.) at any point.

8. Standardization

8.1 *Range:*

8.1.1 The instrument display shall be adjusted using the A-scans for each focal law used to provide an accurate indication of sound travel in the test material. Range standardization shall include correction for wedge travel time so that the zero-depth position in the test piece is accurately indicated for each focal law.

8.1.2 Time base linearity and accuracy shall be verified in accordance with the guidelines in Practice E 2491, or Practice E 317, or both.

8.1.3 Volume-corrected B-scan or S-scan displays shall indicate the true depth to known targets to within 5 % of the physical depth or 3 mm, whichever is less.

8.1.4 Range standardization shall be established using the radius surfaces in reference blocks such as the IIW Block and these blocks shall be made of the same material or acoustically similar material as the test piece.

8.2 *Sensitivity:*

8.2.1 Reference standards for sensitivity-amplitude standardization should be designed so that sensitivity does not vary with beam angle when angle beam testing is used. Sensitivity amplitude reference standards that accomplish this are side-drilled holes parallel to the major surfaces of the plate and perpendicular to the sound path, flat-bottomed holes drilled at the testing angle, and equal-radius reflectors. Surface notches may be used under some circumstances but are not generally recommended.

8.2.2 Standardization shall include the complete ultrasonic phased array system and shall be performed prior to use of the system in the thickness range under examination.

8.2.3 Standardization on reference block(s) shall be performed from the surface (clad or unclad; convex or concave) corresponding to the surface of the component from which the examination will be performed.

8.2.4 The same couplant to be used during the examination shall be used for standardization.

8.2.5 The same contact wedges or immersion/bubbler systems used during the examination shall be used for standardization.

8.2.6 The same focal law(s) used in standardization shall be used for examination.

8.2.7 Any control which affects instrument amplitude response (for example, pulse-duration, filters, averaging, etc.) shall be in the same position for standardization and examination.

8.2.8 Any control which affects instrument linearity (for example, clipping, reject, suppression) shall not be used.

8.2.9 A baseline assessment of element activity shall be made in accordance with Annex A3 of Practice E 2491.

9. Coupling Conditions

9.1 *Preparation:*

9.1.1 Where accessible, prepare the surface of the deposited weld metal so that it merges into the surfaces of the adjacent base materials; however, the weld may be examined in the as-welded condition, provided the surface condition does not interfere with valid interpretation of indications.

9.1.2 Clean the scanning surfaces on the base material of weld spatter, scale, dirt, rust, and any extreme roughness on each side of the weld for a distance equal to several times the thickness of the production material, this distance to be governed by the size of the search unit and refracted angle of the sound beam. Where scanning is to be performed along the top or across this weld, the weld reinforcement may be ground to provide a flat scanning surface. It is important to produce a surface that is as flat as possible. Generally, the surfaces do not

require polishing; light sanding with a disk or belt sander will usually provide a satisfactory surface for examination.

9.1.3 The area of the base material through which the sound will travel in the angle-beam examination should be completely scanned with a straight-beam search unit to detect reflectors that might affect the interpretation of angle-beam results by obstructing the sound beam. Consideration must be given to these reflectors during interpretation of weld examination results, but their detection is not necessarily a basis for rejection of the base material.

9.2 Couplant:

9.2.1 A couplant, usually a liquid or semi-liquid, is required between the face of the search unit and the surface to permit transmission of the acoustic energy from the search unit to the material under examination. The couplant should wet the surfaces of the search unit and the test piece, and eliminate any air space between the two. Typical couplants include water, oil, grease, glycerin, and cellulose gum. The couplant used should not be injurious to the material to be examined, should form a thin film, and, with the exception of water, should be used sparingly. When glycerin is used, a small amount of wetting agent is often added, to improve the coupling properties. When water is used, it should be clean and de-aerated if possible. Inhibitors or wetting agents, or both, may be used.

9.2.2 The coupling medium should be selected so that its viscosity is appropriate for the surface finish of the material to be examined.

9.3 For contact examination, the temperature differential between the reference block and examination surface shall be within 15°C (25°F).

10. Distance-Amplitude Correction

10.1 Reference standards for sensitivity-amplitude standardization should be constructed of materials with similar surface finish, nominal thickness and metallurgically similar in terms of alloy and thermal treatment to the weldment.

10.2 Alternative methods of distance-amplitude of correction of sensitivity may be used provided the results are as reliable as those obtained by the acceptable method. In addition, the alternative method and its equipment shall meet all the performance requirements of this standard.

10.3 Reference Reflectors:

10.3.1 Straight-Beam Standardization—Correction for straight beam examination may be determined by means of a side drilled hole reflector at $\frac{1}{4}$ and $\frac{3}{4}$ of the thickness. For thickness less than 50 mm (2 in.), the $\frac{1}{4}$ -thickness reflector may not be resolved. If this is the case, drill another hole at $\frac{1}{2}$ thickness and use the $\frac{1}{2}$ and $\frac{3}{4}$ -thickness reflectors for correction.

10.3.2 Angle-Beam Standardization—Correction for angle-beam examination may be determined by means of side-drilled hole reflectors at $\frac{1}{4}$ and $\frac{3}{4}$ of the thickness. The $\frac{1}{2}$ -thickness depth to a side-drilled hole may be added to the standardization or used alone at thicknesses less than 25 mm (1 in.). For certain combinations of thin wall and small diameter pipe side drilled holes may not be practical and surface notches may be used with agreement between contracting parties.

10.3.3 The size of the side-drilled hole used for setting sensitivity shall be agreed upon by the contracting parties.

Other targets may be substituted for side-drilled holes if agreed upon by the contracting parties.

10.4 Acceptable Technique:

10.4.1 Time-Corrected Gain—Assessment of phased array examinations uses color-coded B-scans or S-scans as the initial evaluation method. Therefore, it is necessary that the display used provide a uniform color code related to amplitude at all sound path distances. This method can be used only if the instrument is provided with electronic distance amplitude compensation circuitry (TCG). Use is made of all reflectors in the standardization range. The test equipment, probe(s), focal law(s), couplant, etc., to be used in the ultrasonic examination shall be used for this attenuation adjustment.

10.4.2 With the instrument display in time or sound path (not true depth) locate the focal law that provides the maximum response from the reference targets. Set the signal from the reference reflector that gives the highest response, to a screen height of between 40 % to 80 % full screen height (FSH). This target may be considered the primary reference reflector.

10.4.3 Using the same focal law, maximize each of the other reference reflectors at other distances over the range to be used for examination, adjusting the electronic distance amplitude correction controls to equalize the screen height from these reference reflectors to the primary reflector. Apply the correction to all focal laws used for the examination.

10.4.4 Other methods of accomplishing the equalization of amplitude for all focal laws used from equal-size reflectors over the examination distance range may be used. The method for the system used is best described for each instrument in the operating manual for that instrument.

10.4.5 An example of sensitivity standardization for weld examination using side-drilled holes is shown in Fig. 1. Note the amplitude responses from the side drilled holes is the same for each hole even though the angle used to detect the hole and the sound path to the hole is different in each instance. The modeled coverage in the upper portion of Fig. 1 illustrates the beams as if they were projected instead of reflected off the opposite wall. The weld profile overlay allows visualization sound path to the side drilled holes.

10.5 Periodic checks of the sensitivity shall be made at a frequency agreed upon by the contracting parties. If the equipment has changed by more than the agreed upon tolerances, it shall be re-standardized. If the source of sensitivity change is a result of change in the number of active elements compared to the baseline assessment it may require probe replacement.

11. Examination Procedures

11.1 Phased array examination procedures are nominally identical to conventional ultrasonic procedures in coverage, angles etc. Examination procedures recommended for common weld configurations are detailed in Practice E 164. Variations in specifics of the procedures for phased array methods are required depending on whether manual or encoded scanning is used.

11.2 Phased array scanning procedures for welds shall be established using scan plans that indicate the required stand-off positions for the probe to ensure volume coverage required and appropriate beam angles. Volume coverage required may

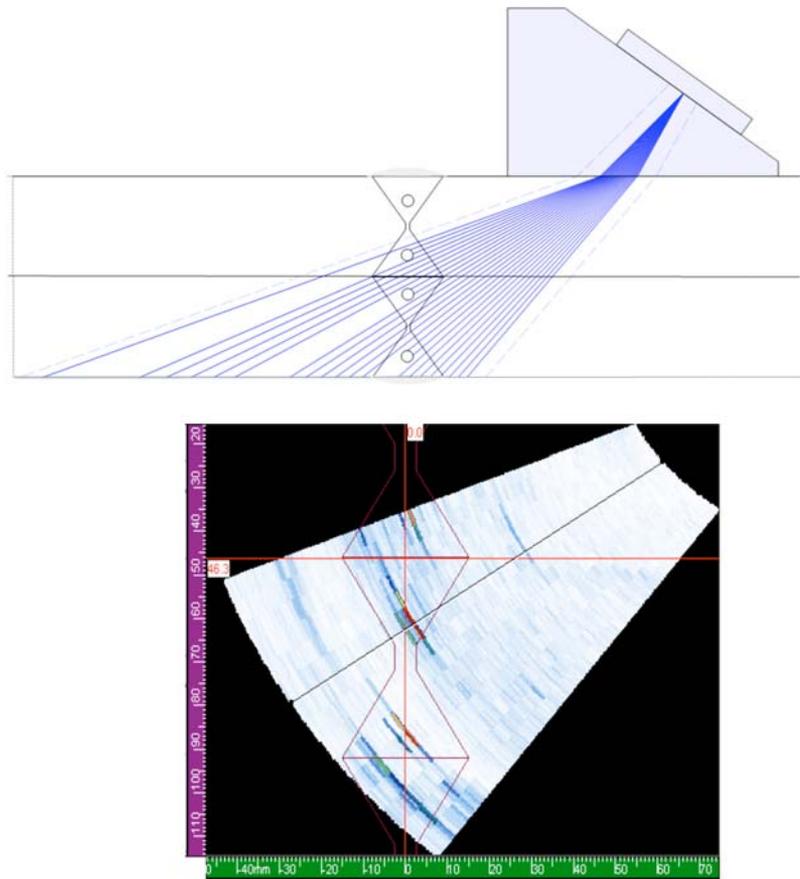


FIG. 1 Modeled S-scan and S-scan Display of Side-Drilled Holes Corrected to 80 % Screen Height Using TCG

include the full volume of weld plus a specified region either side (such as the heat affected zone). Welds shall be inspected from both sides, where possible.


11.3 In addition, if cross-cracking (transverse cracking) is suspected, a supplementary technique shall be used that directs the beam parallel or essentially parallel to the weld centerline. The technique used will depend on whether or not the weld reinforcement has been ground flush or not.

11.4 Typically scanning is carried out from the surfaces where the plate has been machined with the weld bevel. Alternative scanning techniques shall be used for different weld profiles. Sample illustrations are shown in Figs. 2-7. Not all possible configurations are illustrated; illustrations are examples only. Volume coverage afforded by multiple stand-off positions of probes are illustrated for encoded linear scans. This can be replaced with raster scanning where the stand-offs

are continuously varied to the limits required using manual movement of the probes.


11.5 Scanning may be by manual probe motion or automated or semi-automated motion.

11.6 For manual scanning the primary scan pattern is a raster motion with the beam directed essentially perpendicular to the weld axis. The distance forward and backward that the probe is moved is determined by the scan plan to ensure full volume coverage. The lateral movement on each raster step shall not exceed half the element dimension in the lateral direction. Scanning speed (speed at which the probe is manually moved forward and backward) will be limited by the system update capabilities. Generally using more focal laws requires more processing time so update rates of the B-scan or S-scan displays are slower as more focal laws are used.

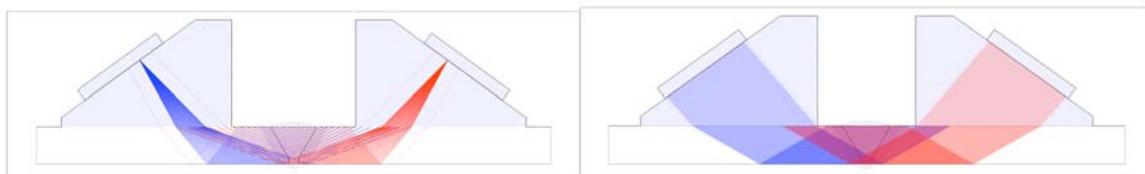


NOTE—Butt welds should be examined from both sides of the weld and preferably from the bevel opening side (when access permits). For thin wall sections, a single probe stand-off may be possible for linear scanning if the probe parameters are adequate for full volume coverage.

FIG. 2 Thin Butt Weld (S and E Scans)

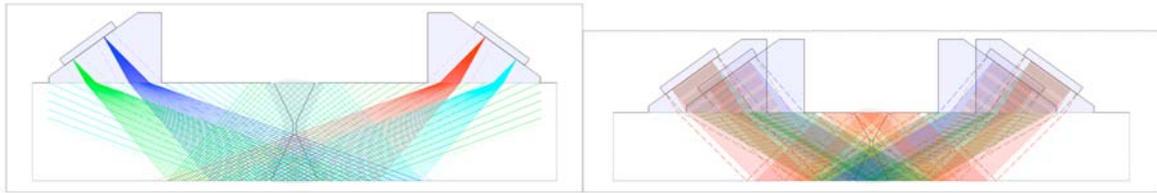


NOTE—Butt welds should be examined from both sides of the weld and preferably from the bevel opening side (when access permits). For thick wall sections, multiple probe stand-offs or multiple focal law stand-offs will be required for linear scanning to ensure full volume coverage.

FIG. 3 Thick Butt Welds (S and E Scans)

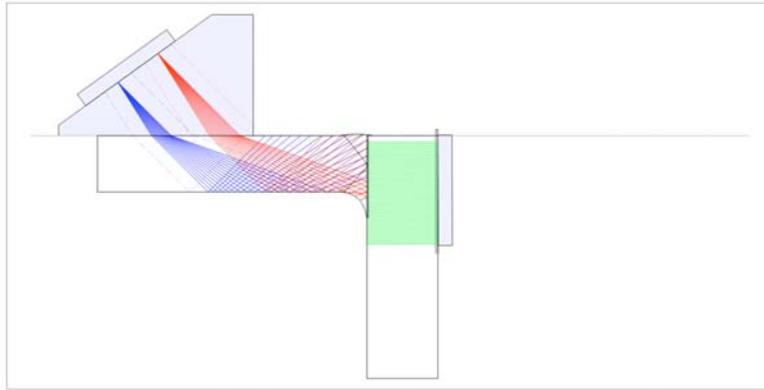


NOTE—Corner welds are to be addressed using a combination of angle beams and straight beams. The preferred probe placement for the angle beam is on the surface where the weld bevel opening occurs. For double Vee welds, angle beam examinations should be carried out from both surfaces when access permits. In most cases, the surface from which the straight beam is used needs no further examination using angle beams.

FIG. 4 Corner Welds (Combined S and E Scans)

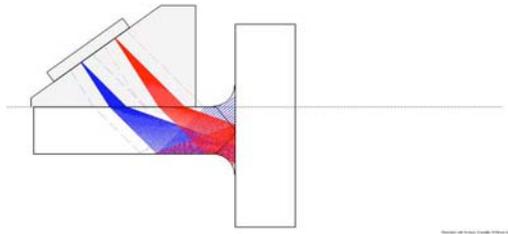

NOTE—T-weld examinations may be treated similarly to butt welds. For thin sections, it may be possible to use a single stand-off position with either E-scans or S-scans. Examination from both surfaces of the web-plate plate should be used when access permits.

FIG. 5 T-Weld (from Web)

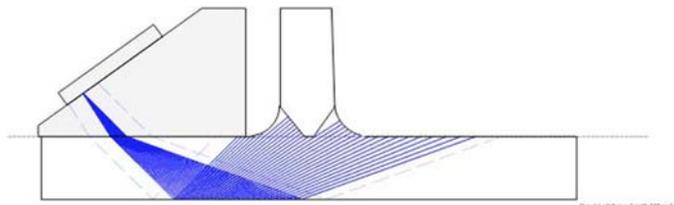


NOTE—An alternative to the technique illustrated in Fig. 5 for T-welds is to use refracted shear wave S-scans or E-scans from web-side of flange surface. More than one stand-off position may be required for thicker sections. Examination from both sides of the web plate should be used when access permits. This technique is not generally considered to be as effective as the technique described in Fig. 5.

FIG. 6 Tee Welds (from Flange)

11.7 For automated or semi-automated scanning the probe will be used with a positional encoder for each axis in which probe motion is required (for most applications a single

encoder is used). The encoder shall be calibrated to provide positional information from a reference start position and shall be accurate to within 1 % of total scan length or 10 mm (0.4

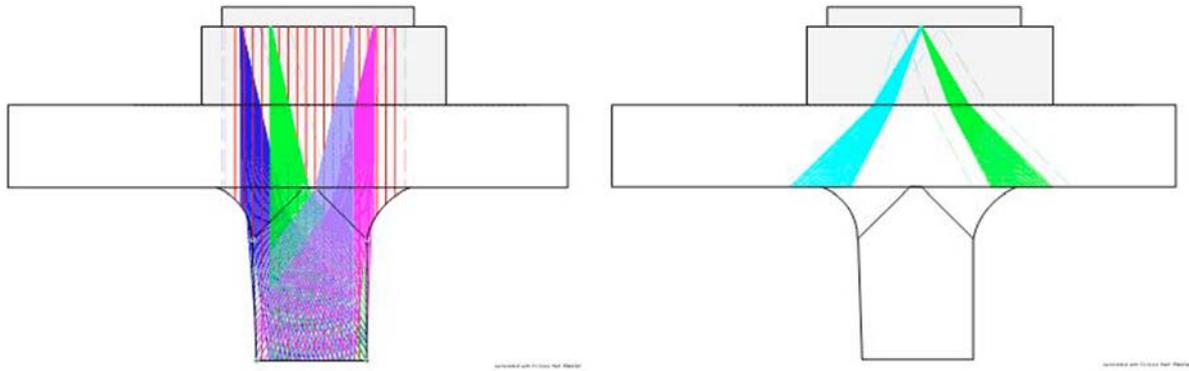

NOTE—When access permits, the preferred technique for T-weld examinations is from the plate opposite the web. A combination of 0° E-scans, and angled compression and shear modes from each direction provides the best approach for flaw detection along the fusion faces of the weld.

FIG. 7 Tee Welds (from Flange Opposite Web)

in.), whichever is less. Guide mechanisms such as probe holding frames or magnetic strips are used to ensure that the probe moves at a fixed distance from the weld centerline. Data, in the form of A-scans from each focal law used, shall be collected at increments of not greater than 2 mm (with at least three increments for the length of the smallest required detectable defect, that is, a defect length of 3 mm would require increments of not greater than 1 mm) along the scan axis. Note that this interval should be reduced when length sizing of flaws is critical with respect to the acceptance criteria. If laterally focused beams are used, this can be considered for data collection increments as above.

11.8 For encoded scanning only, multiple probes and multiple focal law groups (for example, two S-scans from the same probe but having different start elements) may be used simultaneously if the system has the capability. Probe placement will be defined by the details of the scan plan with confirmation of coverage confirmed using notches that may be incorporated into the reference block.

12. Indication Evaluation

12.1 The method of evaluation used, will to some extent, depend on whether manual or encoded scanning was used.

12.2 Manual Scanning:

12.2.1 For manual scanning using phased arrays examination personnel shall use a real-time S-scan or B-scan display during scanning to monitor for coupling quality and signals exceeding the evaluation threshold.

12.2.2 Evaluation of indications detected using manual phased array methods shall require the operator to assess all indications exceeding the evaluation threshold when the indication is detected during the scanning process. Some phased-array systems may include options for entering some items into a report format and incorporating S-scan or B-scan images as part of the report.

12.3 Encoded Scanning:

12.3.1 Encoded scanning methods rely on assessment of data displays produced from stored A-scans.

12.3.2 Encoded systems may be equipped with real-time displays to display one or more views of data being collected during the scan. This feature will be used only for assessment

of data quality as the scan is progressing and may allow for one or more channels to be monitored.

12.3.3 Evaluation of indications detected by encoded phased array scanning shall be made using the digitized waveforms underlying the S-scans or B-scans collected during the data acquisition process.

12.3.4 Encoded scanning data displays for indication evaluation may use a variety of projections other than just the S-scans or B-scans available to manual scanning (for example, top-side-end views).

12.3.5 Welds scanned using encoded techniques may be scanned in sections provided that there is an overlap of data collected and the overlap between scans is identified in the encoded position with respect to the weld reference start position (for example, a 2-m long weld may be scanned in two parts; one from 0 to 1000 mm and the second from 950 to 2000 mm).

12.3.6 The evaluation threshold should be indicated on the S-scan or B-scan display as a well defined color such that indications of note are easily distinguished from the background level.

12.3.7 S-scan or B-scan images presented with angular correction (also referred to as volume corrected) contain signal amplitude and indication depth information projected for the refracted angle of the ultrasonic beam.

12.3.8 Indication locations shall be determined relative to the inspection surface and a coordinate system that uses well defined reference for the relative to the weld.

12.4 Indication Size Determination:

12.4.1 Indication length is generally determined by determining the distance between the points along the weld length where the amplitude drops to half the maximum at the extremities of the reflector, or when the amplitude drops to half the minimum evaluation amplitude.

12.4.2 Estimates of indication height can be made using the 6-dB drop as determined from the S-scan or B-scan (see Fig. 8). This method is suitable for large planar flaws with extents greater than the beam. For flaws with dimensions smaller than the beam a correction for beam divergence may be used to improve sizing estimates. For adversely oriented indications or indications with irregular surfaces, amplitude sizing techniques

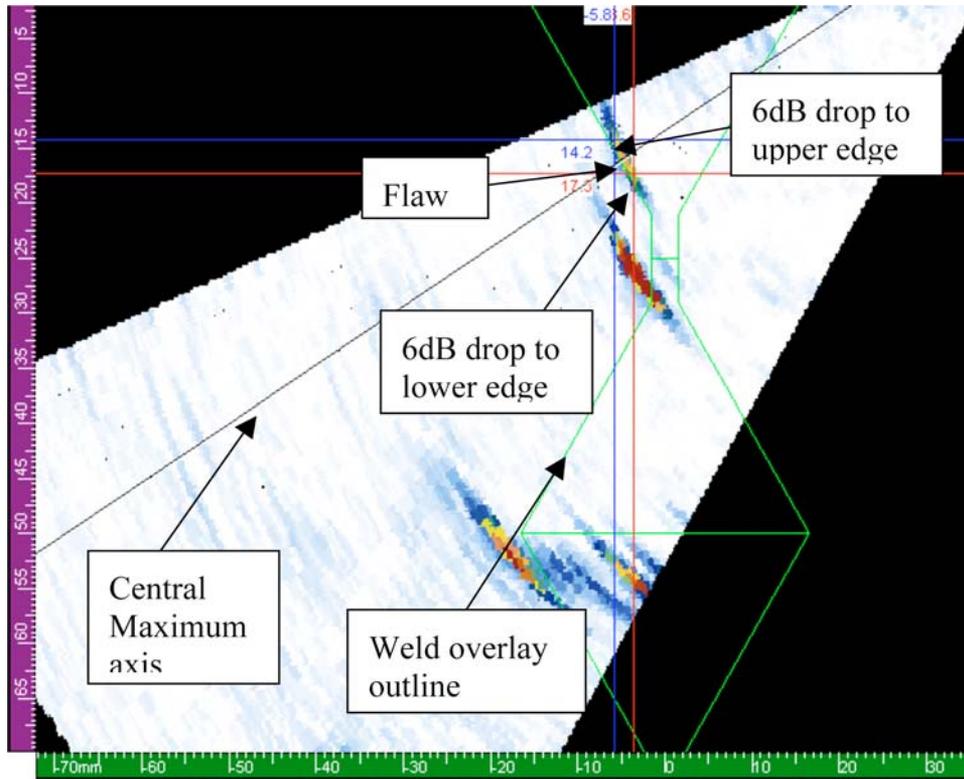


FIG. 8 Flaw Sizing (Vertical) by 6dB Drop

may not accurately indicate size or severity of the indications. For improved sizing capabilities techniques described in Guide E 2192 may be more suitable and can be adapted to phased array applications.

12.4.3 Evaluation of all relevant indications will be made against the acceptance criteria agreed upon by the contracting parties.

13. Reporting

13.1 The contracting parties should determine the pertinent items to be reported. This may include the following information:

13.2 Weld details including thickness dimensions, material, weld process and bevel shape. Descriptive sketches are usually recommended.

13.2.1 Scan surfaces and surface conditions.

13.2.2 *Equipment:*

13.2.2.1 Phased array ultrasonic instrument details.

13.2.2.2 Phased array probe details including:

- (1) Number of elements,
- (2) Frequency,
- (3) Element pitch dimensions,
- (4) Focus (identify plane, depth or sound path as applicable and if applicable),
- (5) Wedge (velocity, incident angle, dimensions, reference dimensions to first element).

13.2.3 Virtual aperture use, that is, number of elements and element width,

13.2.4 Element numbers used for focal laws,

13.2.5 Angular range of S-scan,

13.2.6 Documentation on recommended wedge angular range from manufacturer,

13.2.7 Documented calibration, TCG and angle gain compensation,

13.2.8 Encoder(s),

13.2.9 Scanning mechanisms used,

13.2.10 Couplant,

13.2.11 Method of sensitivity standardization and details of correlating indications with flaws,

13.2.12 Scan plan (indicating probe position on test piece, probe movement, angles used and volume coverage,

13.2.13 Mode of transmission (compression, shear, pulse-echo, tandem, through transmission),

13.2.14 Scanning results (flaw details such as length, position, height, amplitude, acceptability with respect to agreed specifications),

13.2.15 Operator name,

13.2.16 Date of examination.

14. Keywords

14.1 nondestructive testing; phased arrays; phased array probe; ultrasonic contact examination; ultrasonic NDT of welds; welds

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).